



# Influenza A+B Rapid Test Cassette

(Swab/Nasal Aspirate)

## Package Insert

REF IIN-502 English

A rapid test for the qualitative detection of Influenza A and Influenza B virus in nasopharyngeal swab, throat swab or nasal aspirate specimens.

For professional *in vitro* diagnostic use only.

### 【INTENDED USE】

The Influenza A+B Rapid Test Cassette (Swab/Nasal Aspirate) is a rapid chromatographic immunoassay for the qualitative detection of influenza A and B antigens in nasopharyngeal swab, throat swab or nasal aspirate specimens. It is intended to aid in the rapid differential diagnosis of influenza A and B viral infections.

### 【SUMMARY】

Influenza (commonly known as 'flu') is a highly contagious, acute viral infection of the respiratory tract. It is a communicable disease easily transmitted through the coughing and sneezing of aerosolized droplets containing live virus.<sup>1</sup> Influenza outbreaks occur each year during the fall and winter months. Type A viruses are typically more prevalent than type B viruses and are associated with most serious influenza epidemics, while type B infections are usually milder.

The gold standard of laboratory diagnosis is 14-day cell culture with one of a variety of cell lines that can support the growth of influenza virus.<sup>2</sup> Cell culture has limited clinical utility, as results are obtained too late in the clinical course for effective patient intervention. Reverse Transcriptase Polymerase Chain Reaction (RT-PCR) is a newer method that is generally more sensitive than culture with improved detection rates over culture of 2-23%.<sup>3</sup> However, RT-PCR is expensive, complex and must be performed in specialized laboratories.

The Influenza A+B Rapid Test cassette (Swab/Nasal Aspirate) qualitatively detects the presence of Influenza A and/or Influenza B antigen in nasopharyngeal swab or throat swab or nasal aspirate specimens, providing results within 15 minutes. The test uses antibodies specific for Influenza A and Influenza B to selectively detect Influenza A and Influenza B antigen in nasopharyngeal swab, throat swab or nasal aspirate specimens.

### 【PRINCIPLE】

The Influenza A+B Rapid Test Cassette (Swab/Nasal Aspirate) is a qualitative, lateral flow immunoassay for the detection of Influenza A and Influenza B nucleoproteins in nasopharyngeal swab, throat swab or nasal aspirate specimens. In this test, antibodies specific to the Influenza A and Influenza B nucleoproteins is separately coated on the test line regions of the test cassette. During testing, the extracted specimen reacts with the antibodies to Influenza A and/or Influenza B that are coated onto particles. The mixture migrates up the membrane to react with the antibodies to Influenza A and/or Influenza B on the membrane and generate one or two colored lines in the test regions. The presence of this colored line in either or both of the test regions indicates a positive result. To serve as a procedural control, a colored line will always appear in the control region if the test has performed properly.

### 【REAGENTS】

The test cassette contains anti-Influenza A and B particles and anti- Influenza A and B coated on the membrane.

### 【PRECAUTIONS】

Please read all the information in this package insert before performing the test.

1. For professional *in vitro* diagnostic use only. Do not use after the expiration date.
2. The test should remain in the sealed pouch until ready to use.
3. All specimens should be considered potentially hazardous and handled in the same manner as an infectious agent.
4. The used test should be discarded according to local regulations.

### 【STORAGE AND STABILITY】

Store as packaged at room temperature or refrigerated (2-30 °C). The test is stable through the expiration date printed on the sealed pouch. The test must remain in the sealed pouch until use. **DO NOT FREEZE.** Do not use beyond the expiration date.

### 【SPECIMEN COLLECTION AND PREPARATION】

#### • Nasopharyngeal swab sample

1. Insert a sterile swab into the nostril of the patient, reaching the surface of the posterior nasopharynx.

2. Swab over the surface of the posterior nasopharynx 5-10 times.

#### • Throat swab sample

Insert a sterilized swab into pharynx and collect mucocoeperidermis mainly wiping flare region of post-pharyngeal wall and palatine tonsil several times, and be careful not to make saliva attach to the swab.

#### • Nasal aspirate

Connect an aspiration catheter to an aspiration trap that is attached to an aspiration device, insert the catheter to nasal cavity from a nostril, start the aspiration device and then collect nasal aspirate sample. Dip a sterilized swab into the collected nasal aspirate sample and make the specimen cling to the swab.


### 【MATERIALS】

- |                        |                      |                    |
|------------------------|----------------------|--------------------|
| • Test Cassettes       | • Extraction Reagent | • Extraction Tubes |
| • Sterile Swabs        | • Package Insert     | • Workstation      |
| • Extraction Tube Tips |                      |                    |
- Materials required but not provided**
- Timer
  - Aspiration Device

### 【DIRECTIONS FOR USE】

**Allow the test, specimen, extraction buffer to equilibrate to room temperature (15-30 °C) prior to testing.**

1. Remove the test cassette from the sealed foil pouch and use it as soon as possible. Best results will be obtained if the assay is performed immediately after opening the foil pouch.
2. Place the Extraction Tube in the workstation. Hold the extraction reagent bottle upside down vertically. Squeeze the bottle and let the solution drop into the extraction tube freely without touching the edge of the tube. Add **10 drops of extraction reagent** (Approx. 400 µL) to the Extraction Tube. See illustration 1.
3. Place the swab specimen in the Extraction Tube. Rotate the swab for approximately 10 seconds while pressing the head against the inside of the tube to release the antigen in the swab. See illustration 2.
4. Remove the swab while squeezing the swab head against the inside of the Extraction Tube as you remove it to expel as much liquid as possible from the swab. Discard the swab in accordance with your biohazard waste disposal protocol. See illustration 3.
5. Fit the dropper tip on top of the extraction tube. Place the test cassette on a clean and level surface. See illustration 4
6. Add **three drops of the solution** (approx. 120 µL) to the sample well and then start the timer.
7. Wait for the colored line(s) to appear. Read the result at **15 minutes**. Do not interpret the result after 20 minutes.

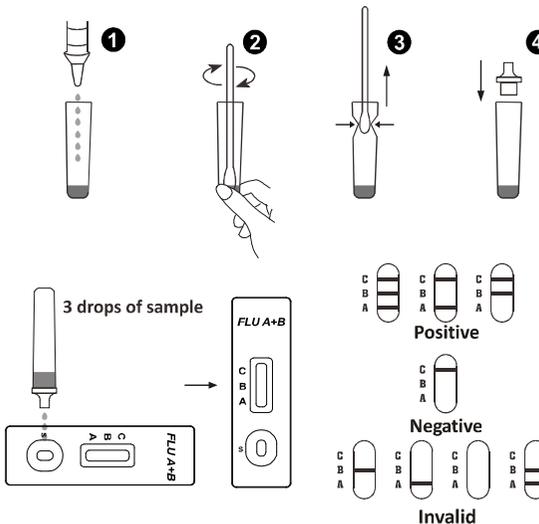

### 【INTERPRETATION OF RESULTS】

(Please refer to the illustration above)

**POSITIVE Influenza A:\*** Two colored lines appear. One colored line should be in the control region (C) and another colored line should be in the Influenza A region (A). A positive result in the Influenza A region indicates that Influenza A antigen was detected in the sample.

**POSITIVE Influenza B:\*** Two colored lines appear. One colored line should be in the control region (C) and another colored line should be in the Influenza B region (B). A positive result in the Influenza B region indicates that Influenza B antigen was detected in the sample.

**POSITIVE Influenza A and Influenza B:\*** Three colored lines appear. One colored line should be in the control region (C) and two colored lines should be in the Influenza A region (A) and Influenza B region (B). A positive result in the Influenza A region and Influenza B region indicates that Influenza A antigen and Influenza B antigen were detected in the sample.

**\*NOTE:** The intensity of the color in the test line regions (A or B) will vary based on the amount of Flu A or B antigen present in the sample. So any shade of color in the test regions (A or B) should be considered positive.

**NEGATIVE: One colored line appears in the control region (C).** No apparent colored line appears in the test line regions (A or B).

**INVALID: Control line fails to appear.** Insufficient specimen volume or incorrect procedural techniques are the most likely reasons for control line failure. Review the procedure and repeat the test with a new test cassette. If the problem persists, discontinue using the test kit immediately and contact your local distributor.

### 【QUALITY CONTROL】

A procedural control is included in the test. A colored line appearing in the control region (C) is the internal procedural control. It confirms sufficient specimen volume and correct procedural technique. Control standards are not supplied with this kit; however, it is recommended that a positive control and a negative control be tested as a good laboratory practice to confirm the test procedure and to verify proper test performance.

### 【LIMITATIONS】

1. The Influenza A+B Rapid Test Cassette (Swab/Nasal Aspirate) is for professional *in vitro* diagnostic use only. The test should be used for the detection of Influenza A and/or B virus in nasopharyngeal swab, throat swab or nasal aspirate specimens. Neither the quantitative value nor the rate of increase in Influenza A and/or B virus concentration can be determined by this qualitative test.
2. The Influenza A+B Rapid Test Cassette (Swab/Nasal Aspirate) will only indicate the presence of Influenza A and/or B virus in the specimen from both viable and non-viable Influenza A and B strains.
3. As with all diagnostic tests, all results must be interpreted together with other clinical information available to the physician.
4. A negative result obtained from this kit should be confirmed by culture. A negative result may be obtained if the concentration of the Influenza A and/or B virus present in the nasopharyngeal swab is not adequate or is below the detectable level of the test.
5. Excess blood or mucus on the swab specimen may interfere with test performance and may yield a false positive result.
6. The accuracy of the test depends on the quality of the swab sample. False negatives may result from improper sample collection or storage.
7. The use of over-the-counter and prescription nasal sprays at high concentrations can interfere with results, leading to either invalid or incorrect test results.
8. A positive result for influenza A and/or B does not preclude an underlying coinfection with another pathogen, therefore the possibility of an underlying bacterial infection should be considered.

### 【EXPECTED VALUES】

The Influenza A+B Rapid Test Cassette (Swab/Nasal Aspirate) has been compared with a leading commercial RT-PCR test. The correlation between these two systems is over 97%.

### 【PERFORMANCE CHARACTERISTICS】

#### Sensitivity, Specificity and Accuracy

The Influenza A+B Rapid Test Cassette (Swab/Nasal Aspirate) has been evaluated with specimens obtained from the patients. RT-PCR is used as the reference method for the Influenza A+B Rapid Test Cassette (Swab/Nasal Aspirate). Specimens were considered positive if RT-PCR indicated a positive result. Specimens were considered negative if RT-PCR indicated a negative result

### Nasopharyngeal Swab Specimen

		Type A			Type B		
		RT-PCR		Total	RT-PCR		Total
		Positive	Negative		Positive	Negative	
Flu A+B	Positive	100	2	102	85	2	87
	Negative	1	180	181	2	200	202
<b>Total</b>		101	182	283	87	202	289
<b>Relative Sensitivity</b>		99.0%			97.7%		
<b>Relative Specificity</b>		98.9%			99.0%		
<b>Accuracy</b>		98.9%			98.6%		

### Throat Swab Specimen

		Type A			Type B		
		RT-PCR		Total	RT-PCR		Total
		Positive	Negative		Positive	Negative	
Flu A+B	Positive	58	1	59	65	1	66
	Negative	3	150	153	4	162	166
<b>Total</b>		61	151	212	69	163	232
<b>Relative Sensitivity</b>		95.1%			94.2%		
<b>Relative Specificity</b>		99.3%			99.4%		
<b>Accuracy</b>		98.1%			97.8%		

### Nasal Aspirate Specimen

		Type A			Type B		
		RT-PCR		Total	RT-PCR		Total
		Positive	Negative		Positive	Negative	
Flu A+B	Positive	46	2	48	94	1	95
	Negative	0	241	241	2	158	160
<b>Total</b>		46	243	289	96	159	255
<b>Relative Sensitivity</b>		100%			97.9%		
<b>Relative Specificity</b>		99.2%			99.4%		
<b>Accuracy</b>		99.3%			98.8%		

### Reactivity with Human Influenza Strain

The Influenza A+B Rapid Test Cassette (Swab/Nasal Aspirate) was tested with the following human influenza strains and a discernible line at appropriate test-line regions was observed:

Influenza A Virus	Influenza B Virus
A/NWS/33 10(H1N1)	B/R5
A/Hong Kong/8/68(H3N2)	B/Russia/69
A/Port Chalmers/1/73(H3N2)	B/Lee/40
A/WS/33(H1N1)	B/Hong Kong/5/72
A/New Jersey/8/76(HswN1)	
A/Mal/302/54(H1N1)	
A/chicken/Yuyao/2/2006 (H5N1)	
A/swine/Hubei/251/2001 (H9N2)	
A/Duck/Hubei/216/1983(H7N8)	
A/Duck/Hubei/137/1982(H10N4)	
A/Anhui/1/2013 (H7N9)	

### Specificity Testing with Various Viral Strains

Description	Test Level
Human adenovirus C	5.62 x 10 <sup>5</sup> TCID <sub>50</sub> /mL
Human adenovirus B	1.58 x 10 <sup>4</sup> TCID <sub>50</sub> /mL
Adenovirus type 10	3.16 x 10 <sup>3</sup> TCID <sub>50</sub> /mL
Adenovirus type 18	1.58 x 10 <sup>4</sup> TCID <sub>50</sub> /mL
Human coronavirus OC43	2.45 x 10 <sup>8</sup> LD <sub>50</sub> /mL
Coxsackievirus A9	2.65 x 10 <sup>4</sup> LD <sub>50</sub> /mL

	1.58 x 10 <sup>5</sup> TCID <sub>50</sub> /mL
Coxsackievirus B5	1.58 x 10 <sup>7</sup> TCID <sub>50</sub> /mL
Human herpesvirus 5	1.58 x 10 <sup>4</sup> TCID <sub>50</sub> /mL
Echovirus 2	3.16 x 10 <sup>5</sup> TCID <sub>50</sub> /mL
Echovirus 3	1 x 10 <sup>4</sup> TCID <sub>50</sub> /mL
Echovirus 6	3.16 x 10 <sup>6</sup> TCID <sub>50</sub> /mL
Herpes simplex virus 1	1.58 x 10 <sup>6</sup> TCID <sub>50</sub> /mL
Human herpesvirus 2	2.81 x 10 <sup>5</sup> TCID <sub>50</sub> /mL
Human Rhinovirus 2	2.81 x 10 <sup>4</sup> TCID <sub>50</sub> /mL
Human Rhinovirus 14	1.58 x 10 <sup>6</sup> TCID <sub>50</sub> /mL
Human Rhinovirus 16	8.89 x 10 <sup>5</sup> TCID <sub>50</sub> /mL
Measles	1.58 x 10 <sup>4</sup> TCID <sub>50</sub> /mL
Mumps	1.58 x 10 <sup>4</sup> TCID <sub>50</sub> /mL
Sendai virus	8.89 x 10 <sup>7</sup> TCID <sub>50</sub> /mL
Parainfluenza virus 2	1.58 x 10 <sup>7</sup> TCID <sub>50</sub> /mL
Parainfluenza virus 3	1.58 x 10 <sup>8</sup> TCID <sub>50</sub> /mL
Respiratory syncytial virus	8.89 x 10 <sup>7</sup> TCID <sub>50</sub> /mL
Human respiratory syncytial virus	1.58 x 10 <sup>5</sup> TCID <sub>50</sub> /mL
Rubella	2.81 x 10 <sup>5</sup> TCID <sub>50</sub> /mL
Varicella-Zoster	1.58 x 10 <sup>5</sup> TCID <sub>50</sub> /mL

TCID<sub>50</sub> = Tissue Culture Infectious Dose is the dilution of virus that under the conditions of the assay can be expected to infect 50% of the culture vessels inoculated.

LD<sub>50</sub> = Lethal Dose is the dilution of virus that under the conditions of the assay can be expected to kill 50% of the suckling mice inoculated.

### Precision

#### Intra-Assay & Inter-Assay

Within-run and Between-run precision has been determined by using five specimens of Influenza standard control. Three different lots of the Influenza Rapid Test Cassette (Swab/Nasal Aspirate) have been tested using negative, Influenza A weak, Influenza B Weak, Influenza A Strong and Influenza B Strong. Ten replicates of each level were tested each day for 3 consecutive days. The specimens were correctly identified > 99% of the time.

#### Cross-reactivity

The following organisms were tested at 1.0x10<sup>8</sup> org/mL and all found to be negative when tested with the Influenza A+B Rapid Test Cassette (Swab/Nasal Aspirate):

<i>Arcanobacterium</i>	<i>Pseudomonas aeruginosa</i>
<i>Candida albicans</i>	<i>Staphylococcus aureus subsp. aureus</i>
<i>Corynebacterium</i>	<i>Staphylococcus epidermidis</i>
<i>Enterococcus faecalis</i>	<i>Staphylococcus saprophyticus</i>
<i>Enterococcus faecium</i>	<i>Streptococcus agalactiae</i>
<i>Escherichia coli</i>	<i>Streptococcus bovis</i>
<i>Haemophilus</i>	<i>Streptococcus dysgalactiae / subsp. dysgalactiae</i>
<i>Moraxella catarrhalis</i>	<i>Streptococcus oralis</i> formerly <i>Streptococcus</i>
<i>Neisseria gonorrhoeae</i>	<i>Streptococcus pneumoniae</i>
<i>Neisseria lactamica</i>	<i>Streptococcus pyogenes</i>
<i>Neisseria subflava</i>	<i>Streptococcus salivarius</i>
<i>Proleus vulgaris</i>	<i>Streptococcus sp group F.type 2</i>

### [BIBLIOGRAPHY]

- Williams, KM, Jackson MA, Hamilton M. (2002) Rapid Diagnostic Testing for URIs in Children; Impact on Physician Decision Making and Cost. *Infect. Med.* 19(3): 109-111.
- Betts, R.F. 1995. Influenza virus, p. 1546-1567. In G.L. Mandell, R.G. Douglas, Jr. and J.E. Bennett (ed.), *Principle and practice of infectious diseases*, 4th ed. Churchill Livingstone, Inc., New York, N.Y.
- WHO recommendations on the use of rapid testing for influenza diagnosis, World Health Organisation, July 2005.

	Consult Instructions for Use		Tests per kit		Authorized Representative
	For <i>in vitro</i> diagnostic use only		Use by		Do not reuse
	Store between 2-30 °C		Lot Number		Catalog #
	Do not use if package is damaged		Manufacturer		

**Hangzhou AllTest Biotech Co.,Ltd.**  
 #550, Yin Hai Street  
 Hangzhou Economic & Technological Development Area  
 Hangzhou, 310018 P.R. China  
 Web: www.alltests.com.cn Email: info@alltests.com.cn



**EC REP**  
 MedNet EC-REP GmbH  
 Borkstrasse 10,  
 48163 Muenster,  
 Germany



Innova Medical Group by  
 Suite 310  
 Grote Bickersstraat 74-78 1013  
 KS, Amsterdam  
 The Netherlands

Service Clients / Customer Service  
 Tel. : +33 (0)1 87 20 01 25  
 Email : commercial@innovamedgroup.com

Number: 146792700  
 Effective date: 2022-06-06